

**TEST REPORT**

CIN - U74220DL1998PLC092698

Issued To: RUST X  
121 SECTOR-5  
IMT MANESAR

GURGOAN


Phone/Fax:  
Kind Attn.: MS. RENU

Sample Description:  
EVA BAG.

Report No.: 150921040/1509210132

Date: 25-Sep-2015  
DCR: 21-Sep-2015

Your Ref. No.:

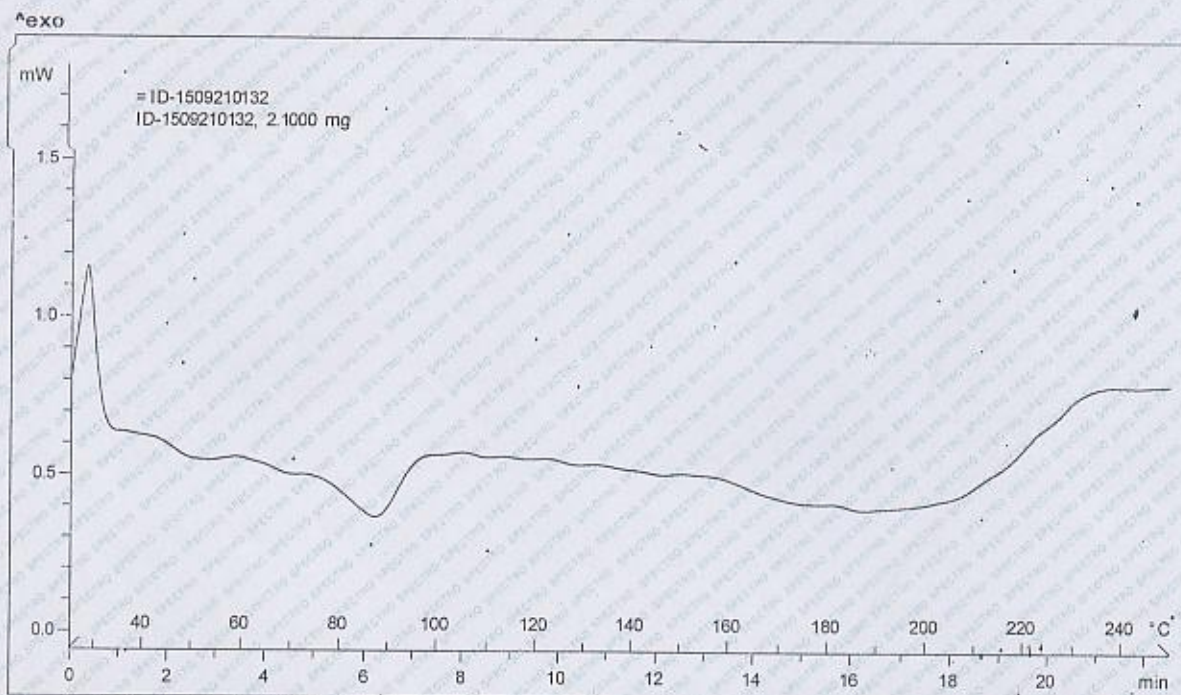

Spectro Analytical Labs Ltd: METTLER

STAR<sup>®</sup> SW 9.10

ID-1509210132

S.NO	Name of Test	Result	Test Method
1.	<u>Differential Scanning Calorimetry (DSC)</u>		ISO:11357(Pt3) -1999
	Melting Peak Temperature, °C	87	

\*\*\*\*\* End of test Report \*\*\*\*\*

*Analyst*  
Analyst



Authorised Signatory

TRA - 199765

CCREQD\1\RA000\JA3420

BIS, DGS & D, DDA, MOEF, DGCA approved,  
ISO - 9001: 2008, ISO 14001 : 2004 & OHSAS 18001:2007 Certified Laboratory  
CIN : U74220DL 1998 PLC 092698  
Subject to Terms & Conditions Overleaf